
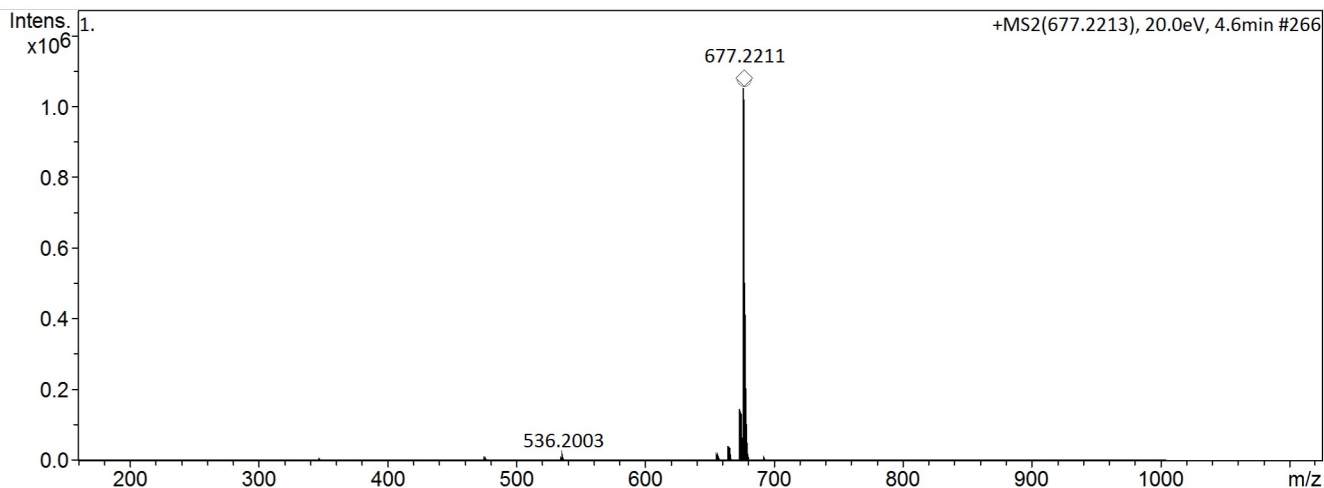
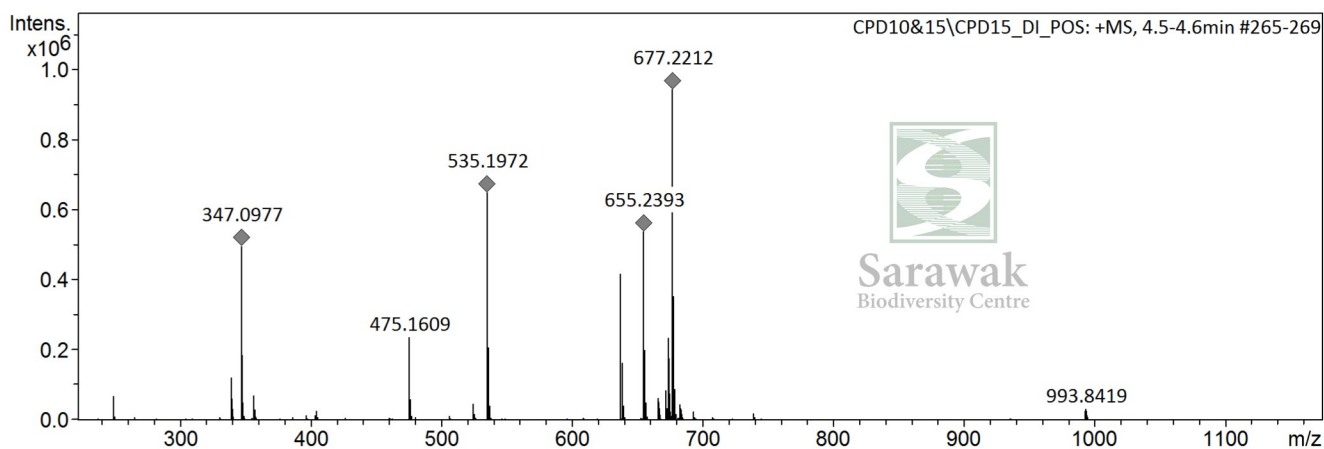


Compound Spectrum SmartFormula Report

Analysis Info

Acquisition Date 10/13/2016 3:03:45 PM
Method flow_injection_pos_160321.ms.ms.m
Sample Name CPD10&15\CPD15_DI_POS

Operator KREd
Instrument impact II

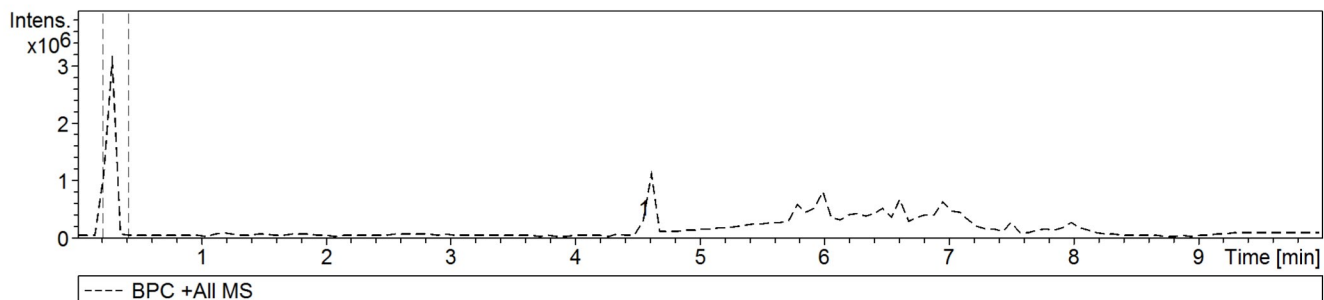

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdb	e ⁻ Conf	N-Rule
677.2211	1	C ₃₄ H ₃₈ NaO ₁₃	677.2205	-1.0	13.0	1	100.00	15.5	even	ok