
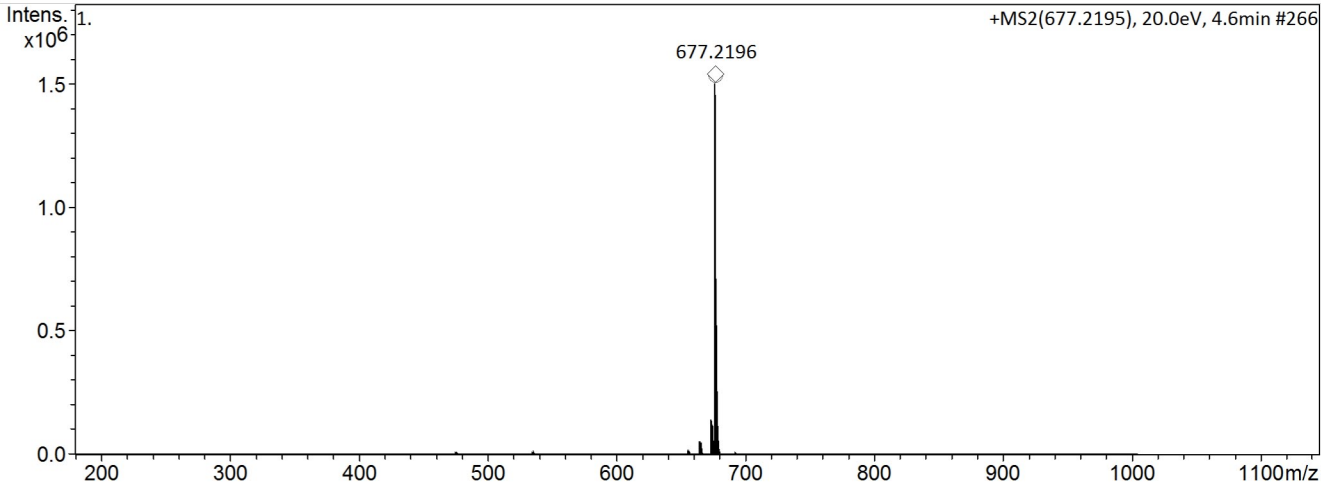
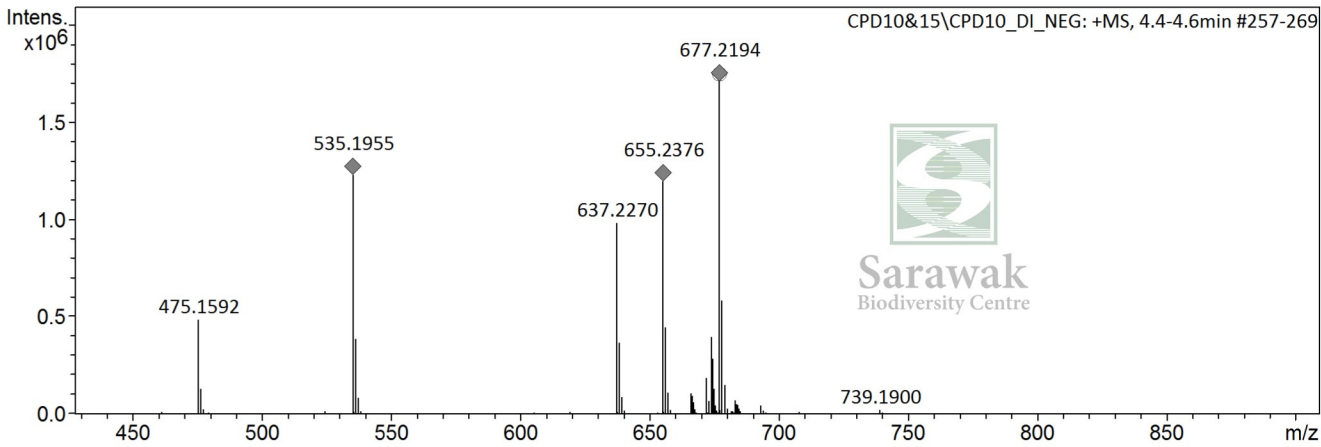


Compound Spectrum SmartFormula Report

Analysis Info

Acquisition Date 10/13/2016 12:55:19 PM
Method flow_injection_pos_160321.ms.ms.m
Sample Name CPD10&15\CPD10_DI_NEG

Operator KREd
Instrument impact II

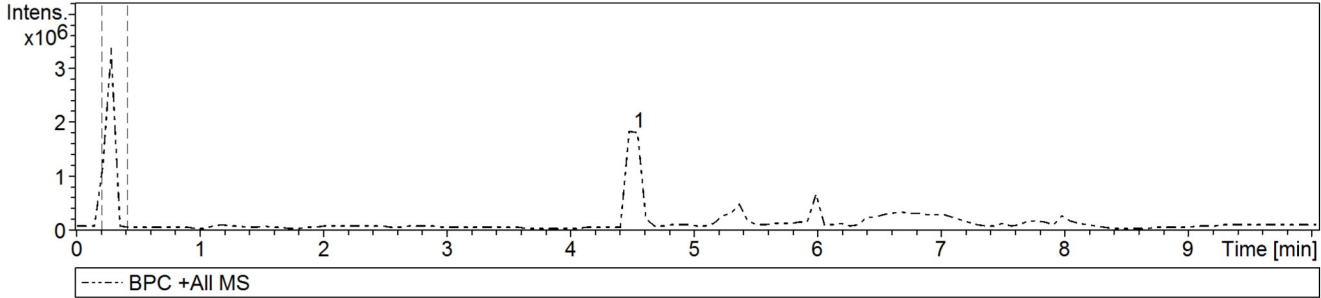

| Meas. m/z | # | Ion Formula | m/z | err [ppm] | mSigma | # mSigma | Score | rdb | e ⁻ Conf | N-Rule |
|-----------|---|---|----------|-----------|--------|----------|--------|------|---------------------|--------|
| 677.2196 | 1 | C ₃₄ H ₃₈ NaO ₁₃ | 677.2205 | 1.3 | 11.4 | 1 | 100.00 | 15.5 | even | ok |